

## **Mining Property for Option**

**Contact: Andre Dugas**

Email: [andreandchantal@parolink.net](mailto:andreandchantal@parolink.net)

Tel./Fax 705.647.5280

Location: Cobalt, Ontario

Parcel #: 5323-5324-3727-3728

Walk in Drift with laid tracks, 6 levels, hydro 550 volts all electrical installed with lighting. All claims have incline adjoining each other, recently did some diamond drilling on property. Good results, core on hand for viewing.

Also Silver Concentrate available – high percentage, (44) drums ready for refinery. Four drums of very high silver (assays follow)



Established 1928

# Swastika Laboratories Ltd

Assaying - Consulting - Representation

## Assay Certificate

Company: **ANDRE DUGAS**  
Project: **COBALT**  
Attn:

**9W-3144-RA1**

Date: OCT-26-09

We hereby certify the following Assay of 2 COARSE SAND samples submitted OCT-19-09 by . . .

Sample Number	Ag oz/ton	Co %	Ni %	Multi Element
D-25-09	80.27	4.47	2.08	RESULTS
D-26-09	87.65	3.75	2.11	TO FOLLOW

Certified by



Established 1928

# Swastika Laboratories Ltd

Assaying - Consulting - Representation

## Assay Certificate

Company: **ANDRE DUGAS**  
Project: **COBALT AREA**  
Attn:

**9W-2996-RA1**

Date: OCT-09-09

We hereby certify the following Assay of 4 MILL SAMPLES samples submitted OCT-02-09 by .

Sample Number	Ag oz/ton	Multi Element
002-D-1-H	67.29	RESULTS
002-D-1-H MIX	67.75	TC
003-D-2-L	70.20	FOLLOW
003-D 2-L MIX	79.33	

Certified by Dennis Chatter

Assayers Canada

8282 Sherbrooke St., Vancouver, B.C., V5X 4R6

Tel: (604) 327-3436 Fax: (604) 327-3423

Report No : 9W2996RJ

Date : Oct-21-09

Andre Dugas

Attention:

Project: Cobalt Area

Sample type: Mill Samples

Multi-Element ICP-AES Analysis

Aqua Regia Digestion

Sample Number	Ag ppm	Al %	As ppm	Ba ppm	Be ppm	Bi ppm	Ca %	Cd ppm	Co ppm	Cr ppm	Cu ppm	Fe %	Hg ppm	K %	La ppm	Mg %	Mn ppm	Mo ppm	Na %	Ni ppm	P ppm	Pb ppm	S %	Sb ppm	Sc ppm	Sr ppm	Th ppm	Ti %	Tl ppm	U ppm	V ppm	W ppm	Zn ppm	Zr ppm
002-D-1-H	>200.0	1.34	>10000	44	0.8	2007	3.04	<1	>10000	55	6497	6.56	4548	0.08	11	1.28	1124	65	0.08	>10000	286	4237	3.13	1057	5	39	10	0.02	<10	34	53	<10	1446	15
002-D-1-H MIX	>200.0	1.33	>10000	38	0.7	2059	2.97	<1	>10000	55	6129	6.61	5398	0.08	11	1.26	862	66	0.08	>10000	292	4098	3.21	809	5	35	9	0.02	<10	28	54	<10	1618	14
003-D-2-L	>200.0	1.36	>10000	52	0.5	1838	2.88	<1	>10000	56	6437	8.15	9568	0.08	11	1.28	1035	66	0.06	>10000	293	4002	2.87	790	5	33	9	0.02	<10	30	53	<10	1584	15
003-D 2-L MIX	>200.0	1.32	>10000	52	0.7	1612	2.76	10	>10000	57	6318	7.88	7894	0.07	11	1.21	922	61	0.06	>10000	273	3776	2.77	803	5	32	9	0.02	<10	28	52	<10	1582	16
<b>Duplicates:</b>																																		
002-D-1-H	>200.0	1.33	>10000	46	0.7	1945	3.18	<1	>10000	56	6472	6.78	4716	0.08	11	1.31	1124	62	0.08	>10000	275	4467	3.23	1070	5	38	10	0.02	<10	35	54	<10	1476	14
<b>Standards:</b>																																		
Blank	<0.2	<0.01	<5	<10	<0.5	<5	<0.01	<1	<1	<1	<1	<0.01	<1	0.01	<10	<0.01	<5	<2	0.01	1	<10	<2	<0.01	<5	<1	<1	<5	<0.01	<10	<10	<1	<10	<1	<1
ICP-5	23.5	1.06	1457	162	<0.5	52	2.03	19	19	181	2158	3.46	1	0.18	<10	1.23	639	7	0.08	116	570	2464	1.15	184	3	64	<5	0.07	<10	<10	64	10	1511	4

A .5 gm sample is digested with 5 ml 3:1 HCl/HNO3 at 95°C for 2 hours and diluted to 25ml.

Signed: \_\_\_\_\_



**Assayers Canada**

8282 Sherbrooke St., Vancouver, B.C., V5X 4R6

Tel: (604) 327-3436 Fax: (604) 327-3423

Report No : 9W3144RJ

Date : Nov-09-09

**Andre Dugas**

Attention:

Project: Cobalt

Sample type: Coarse Sand


**Multi-Element ICP-AES Analysis**

Aqua Regia Digestion

Sample Number	Ag ppm	Al %	As ppm	Ba ppm	Be ppm	Bi ppm	Ca %	Cd ppm	Co ppm	Cr ppm	Cu ppm	Fe %	Hg ppm	K %	La ppm	Mg %	Mn ppm	Mo ppm	Na %	Ni ppm	P ppm	Pb ppm	S %	Sb ppm	Sc ppm	Sr ppm	Th ppm	Ti %	Tl ppm	U ppm	V ppm	W ppm	Zn ppm	Z ppm
D-25-09	>200.0	1.37	>10000	46	0.6	2003	2.93	<1	>10000	85	5546	6.28	4189	0.08	11	1.35	812	106	0.08	>10000	256	5091	3.17	1403	6	36	15	0.03	17	32	64	<10	1227	
D-26-09	>200.0	1.49	>10000	62	0.7	1735	2.84	<1	>10000	101	5981	6.13	8392	0.09	11	1.34	970	105	0.09	>10000	290	3741	2.77	865	6	39	14	0.03	13	30	66	33	1930	
<b>Duplicates:</b>																																		
D-25-09	>200.0	1.37	>10000	45	0.6	2024	2.89	<1	>10000	84	5484	6.28	4092	0.08	11	1.33	790	103	0.08	>10000	250	5402	3.10	1474	6	35	15	0.03	16	31	63	<10	1201	
<b>Standards:</b>																																		
Blank	<0.2	<0.01	<5	<10	<0.5	<5	<0.01	<1	<1	<1	1	<0.01	<1	<0.01	<10	<0.01	<5	<2	<0.01	<1	<10	<2	<0.01	<5	<1	<1	<5	<0.01	<10	<10	<1	<10	<1	
CH-1	1.4	1.81	18	286	<0.5	22	0.59	3	28	104	1934	4.67	2	1.32	13	1.22	326	2	0.06	53	662	21	0.57	9	7	8	<5	0.20	<10	<10	81	<10	209	

A .5 gm sample is digested with 5 ml 3:1 HCl/HNO3 at 95°C for 2 hours and diluted to 25ml.



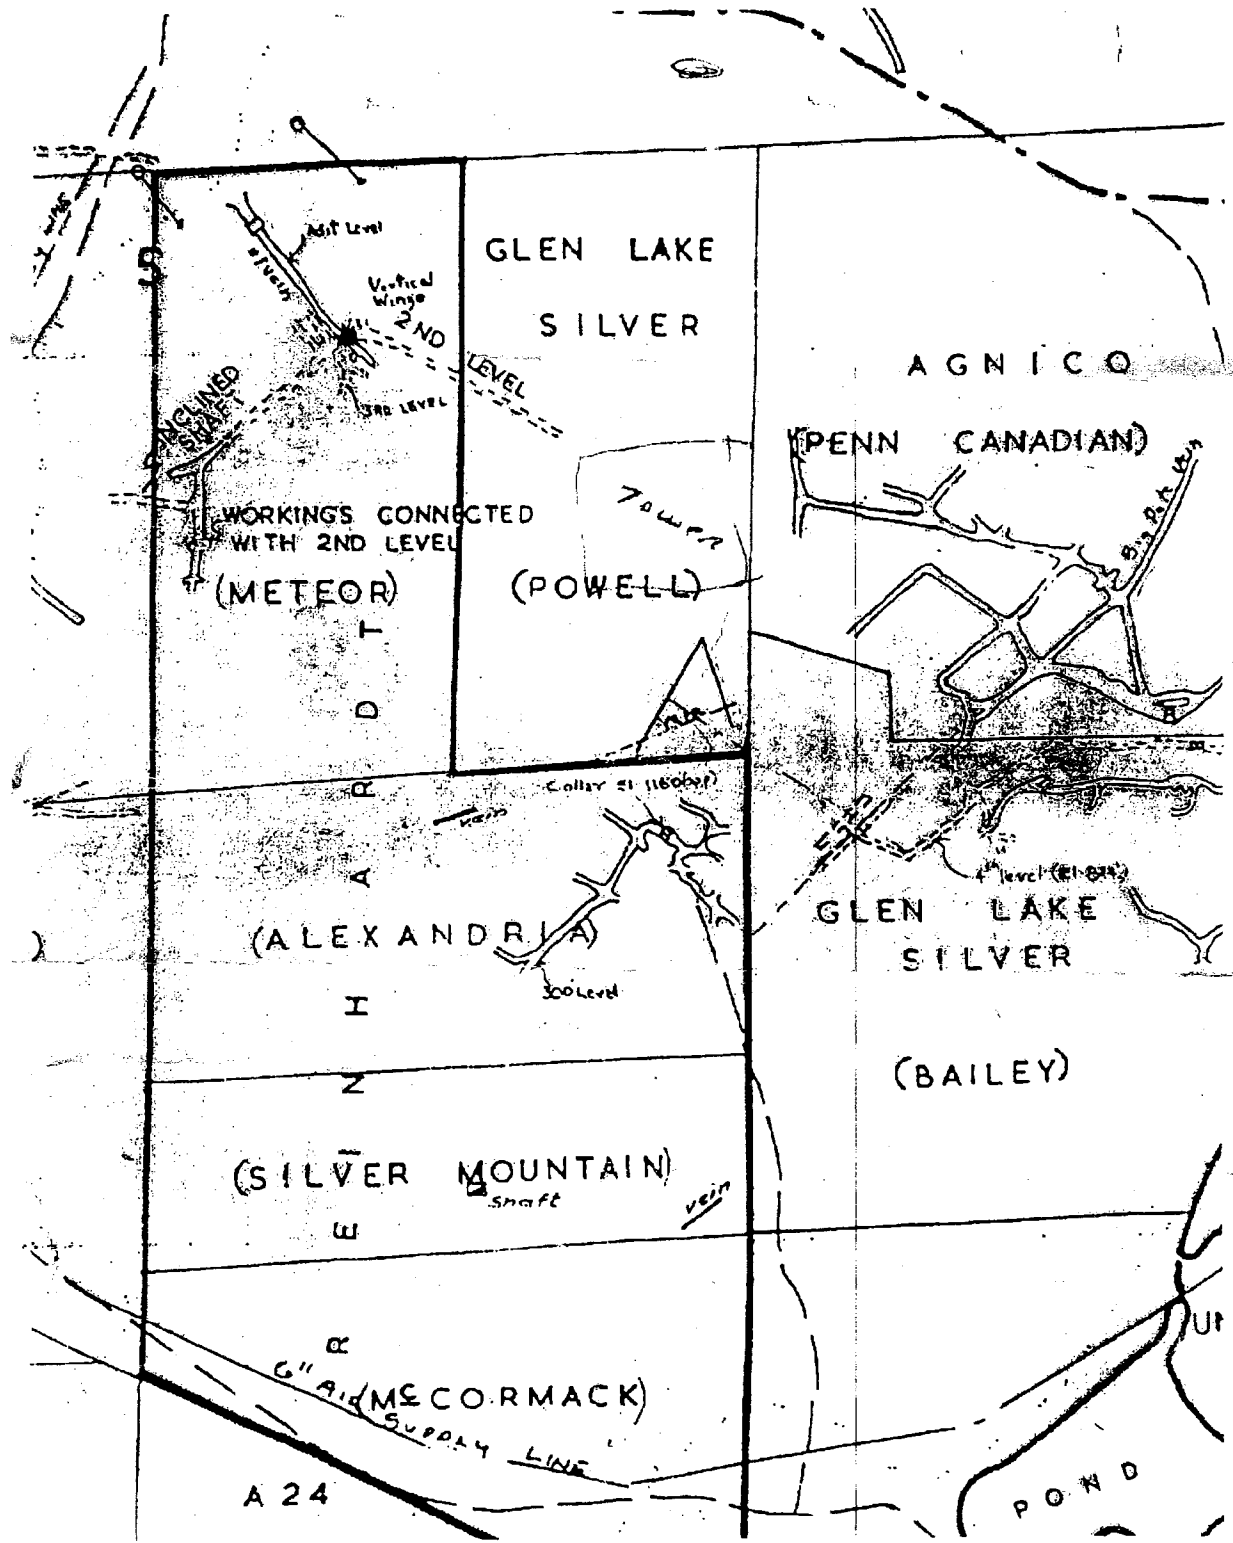

A 24